


如何检查血压计是否通过了规范的准确性检测



为什么需要使用准确的血压计?

不正确的血压测量可能会导致错误的诊断和不恰当的治疗。并且可能会错过早期预防心脏病发作或中风的时机。



存在许多不准确的血压计

可以使用的血压计有 3000 多种, 但只有不到 15% 的血压计通过规范的准确性检测。

仅使用以下(免费)注册中心推荐的血压计

选择您所在国家的注册表, 或者选择一个通用的注册表

特定国家的注册表

点击相应的国家并按照其说明进行操作

[英国](#)

[爱尔兰](#)

[加拿大](#)

[德国](#)

[日本](#)

[美国](#)

常规登记

STRIDE BP

<https://stridebp.org/bp-monitors>

是经过验证的血压计的注册表。请按照第2页的关于如何搜索此注册表的详细说明进行操作。

Medaval

medaval.ie/blood-pressure-monitors/

同时列出了经过验证的和未经验证的血压计。请按照第3页的关于如何搜索此注册表的详细说明进行操作。


如何使用STRIDE BP 注册表检查血压计 是否通过规范的准 确性检测



分步操作指南


01 类型。

在浏览器输入：<https://stridebp.org/bp-monitors>




02 搜索。

通过在搜索框中输入血压计的精确型号。
或者，输入血压计的制造商名称并下拉显示栏找到列出的血压计型号。



如果“设备描述”栏显示该血压计，则表明它已**通过验证**。

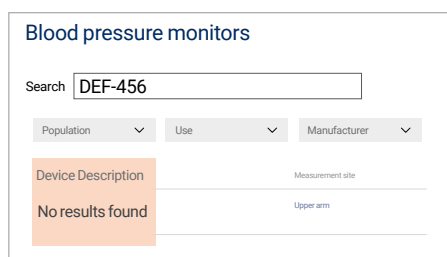

如果“设备描述”栏显示“未找到结果”，则该血压计**未通过验证，不应使用**。



提示：

搜索功能非常灵敏。任何关于血压计制造商名称或型号的小错误都将使**即使已经通过验证**的血压计不能被找到。



提示：

如果未显示血压计的制造商名称或型号，**该血压计不可能是通过验证的**。计不能被找到。

不要被品牌，价格或评论所吸引


如何使用Medaval 注册表检查血压计是否 通过规范的准确性检测



分步操作指南


01 搜索。

使用必应国内版 (cn.Bing.com) *输入血压计的品牌和型号, 以及“Medaval”一词。*或任何其他搜索引擎



02 查找。

查找并单击带有“Medaval”血压计评估的链接。忽略可能出现的任何其他广告。



03 检查。

下拉滚动条至准确性评估报告。找到“Medaval”的对血压计的评估和建议。

Assessment:	The technology used in the Brand X ABC-123 , to measure blood pressure, has passed in a clinical validation study, in a general population, according to a recognised standard protocol, as published in a peer-reviewed publication.		
	Accuracy Assessment	Recommendation	Basis
	Medaval	★★ Recommendation	Recent clinical validation; recent protocol



提示:

如果未显示血压计的制造商名称或型号, 该血压计不可能是通过验证的。



提示:

“Medaval”使用了不同的星级评定, 但任何通过验证的血压计都被推荐使用, 无论其星数多少。

不要被品牌, 价格或评论所吸引

